



INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification 6 : A61L	A2	(11) International Publication Number: WO 99/11296 (43) International Publication Date: 11 March 1999 (11.03.99)
<p>(21) International Application Number: PCT/EP98/05440</p> <p>(22) International Filing Date: 27 August 1998 (27.08.98)</p> <p>(30) Priority Data: 08/921,533 2 September 1997 (02.09.97) US</p> <p>(71) Applicant: BIONX IMPLANTS OY [FI/FI]; Runeberginkatu 3 Al, FIN-33710 Tampere (FI).</p> <p>(72) Inventors: TORMÄLÄ, Pertti; Nestori Sarrin katu 1, FIN-33720 Tampere (FI). KELLOMAKI, Minna; Kasvi- tarhankatu 8, FIN-33500 Tampere (FI). BONFIELD, William; 48 Harner Green Lane, Digswell, Welwyn, Hertfordshire (GB).</p> <p>(74) Agent: KEIL & SCHAAFHAUSEN; Eysseneckstrasse 31, D-60322 Frankfurt am Main (DE).</p>	<p>(81) Designated States: AU, CA, JP, European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE).</p> <p>Published <i>Without international search report and to be republished upon receipt of that report.</i></p>	
<p>(54) Title: BIOACTIVE AND BIODEGRADABLE COMPOSITES OF POLYMERS AND CERAMICS OR GLASSES AND METHOD TO MANUFACTURE SUCH COMPOSITES</p>		
<p>(57) Abstract</p> <p>Surgical osteosynthesis composite material which has three components: biodegradable polymer reinforcement, bioceramic or bioglass filler reinforcement and biodegradable polymer matrix. This invention relates to biodegradable materials used for bone fracture fixation devices and methods of their manufacture. Unlike other known materials used prior to this application, the composites of this invention have two different reinforcing phases and one matrix phase. One reinforcing element is referred as the polymeric reinforcing element and the other as the ceramic reinforcing element.</p> <div data-bbox="429 751 823 909"> </div> <div data-bbox="429 1063 780 1089"> <p>○ Fibrillated polymer reinforcement</p> </div> <div data-bbox="420 1126 844 1163"> <p>■ Mixture of matrix polymer and bioceramic or glass</p> </div>		

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina	GE	Georgia	MD	Republic of Moldova	TG	Togo
BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN	Guinea	MK	The former Yugoslav Republic of Macedonia	TM	Turkmenistan
BF	Burkina Faso	GR	Greece	ML	Mali	TR	Turkey
BG	Bulgaria	HU	Hungary	MN	Mongolia	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MR	Mauritania	UA	Ukraine
BR	Brazil	IL	Israel	MW	Malawi	UG	Uganda
BY	Belarus	IS	Iceland	MX	Mexico	US	United States of America
CA	Canada	IT	Italy	NE	Niger	UZ	Uzbekistan
CF	Central African Republic	JP	Japan	NL	Netherlands	VN	Viet Nam
CG	Congo	KE	Kenya	NO	Norway	YU	Yugoslavia
CH	Switzerland	KG	Kyrgyzstan	NZ	New Zealand	ZW	Zimbabwe
CI	Côte d'Ivoire	KP	Democratic People's Republic of Korea	PL	Poland		
CM	Cameroon	KR	Republic of Korea	PT	Portugal		
CN	China	KZ	Kazakhstan	RO	Romania		
CU	Cuba	LC	Saint Lucia	RU	Russian Federation		
CZ	Czech Republic	LI	Liechtenstein	SD	Sudan		
DE	Germany	LK	Sri Lanka	SE	Sweden		
DK	Denmark	LR	Liberia	SG	Singapore		
EE	Estonia						

**BIOACTIVE AND BIODEGRADABLE COMPOSITES OF
POLYMERS AND CERAMICS OR GLASSES AND
METHOD TO MANUFACTURE SUCH COMPOSITES**

Field of the Invention

The present invention relates to a surgical osteosynthesis composite material, which is biodegradable and bioactive, and methods of manufacturing the composite material.

5

Background of the Invention

In surgery, either biostable or biodegradable devices are used for the fixation of bone fractures to immobilize the bone fragments and accelerate patient mobilization.

10 Most biostable devices are typically made of metallic alloys. See R.M. Pilliar, Powder Metal-Made Orthopaedic Implants With Porous Surface For Fixation By Tissue Ingrowth, Clinical Orthopaedics and Related Research, Vol. 176, 1983, pp. 42-51. Nevertheless, there are several disadvantages in the use of metallic implants. One such disadvantage is bone resorption caused by bone plates and screws, which
15 carry most of the external loads, leading to stress protection produced by the

modulus mismatch between metals and bone. Another disadvantage is the carcinogenic potential and the possibility of corrosion. Therefore, surgeons are recommended to remove metallic bone plates and screws in a second operation once the fracture has healed.

- 5 Bioresorbable polymeric fracture fixation devices have been studied as replacements for metallic implants. *See* S. Vainiopää, P. Rokkanen, P. Törmälä, Surgical Applications Of Biodegradable Polymers In Human Tissue, Progress in Polymer Science, Vol. 14, 1989, pp. 679-716. The advantages of these devices are that materials resorb in the body and degradation products disappear via metabolic
- 10 routes. Hence, a second operation is not required. Additionally, the strength and the stiffness of the bioresorbable polymeric devices decreases when the device degrades and hence the bone is progressively loaded (which promotes bone regeneration). One disadvantage is the relatively low strength of existing polymeric devices. In the case of cortical, bone fracture, for example, unreinforced poly lactic acid (PLLA)
- 15 plate and screws are too weak initially to permit patient mobilization. *See* J. Eitenmüller, K.L. Gerlach, T. Schmickal, H. Krause, An In Vivo Evaluation Of A New High Molecular Weight Polylactide Osteosynthesis Device, European Congress on Biomaterials, Bologna Italy, September 14-17, 1986, p. 94. In addition, the relatively low values of Young's modulus compared to metallic plates mean that
- 20 thicker sections are required to ensure adequate stability.

Törmälä et al. have developed self-reinforced bioresorbable polymeric composites to improve the strength of bioresorbable polymer devices. These show good mechanical properties: e.g. bending strengths of 360 ± 70 MPa and bending moduli of 12 ± 2 GPa, respectively, have been reported. *See* P. Törmälä,

Biodegradable Self-Reinforced Composite Materials; Manufacturing, Structure and Mechanical Properties, Clinical Materials, Vol. 10, 1992, pp. 29-34.

A common property of most polymeric implants is the lack of bony ongrowth to the material. In contrast, such bone apposition is produced by bioactive ceramics and glasses. See O.H. Andersson, K.H. Karlsson, Bioactive Glass, Biomaterials Today And Tomorrow, Proceedings of the Finnish Dental Society Days of Research, Tampere, Finland, 10-11 November 1995, Gillot Oy, Turku, 1996, pp. 15-16. By adding bioactive ceramics or glasses to polymers to produce a composite, the bioactivity of the material can be improved. This effect has been demonstrated in dental composites and bone cement. See J.C. Behiri, M. Braden, S.N. Khorashani, D. Wiwattanadate, W. Bonfield, Advanced Bone Cement For Long Term Orthopaedic Applications, Bioceramics, Vol. 4, ed. W. Bonfield, G.W. Hastings and K.E. Tanner, Butterworth-Heinemann Ltd, Oxford, 1991, pp. 301-307.

Bonfield et al have developed a biostable composite consisting of a polyethylene matrix and a particulate hydroxyapatite reinforcement (HAPEX™). See W. Bonfield, J.A. Bowman, M.D. Gryn timer, UK Patent GB2085461, 1984. HAPEX™ composites show bioactivity above 0.20 volume fraction hydroxyapatite. See W. Bonfield, C. Doyle, K.E. Tanner, In Vivo Evaluation Of Hydroxyapatite Reinforced Polyethylene Composites, Biological and Biomechanical Properties of Biomaterials, ed., P. Crystel, A. Meunter, A.J.C. Lee, Elsevier Science Publisher, 1986, pp. 153-158. Additionally, degradable composites of hydroxyapatite and copolymers of polyhydroxybutyrate and polyhydroxyvalerate have been described. See C. Doyle, K.E. Tanner, W. Bonfield, In Vitro And In Vivo Evaluation Of Polyhydroxybutyrate And Of Polyhydroxyvalerate Reinforced With Hydroxyapatite,

Biomaterials, Vol. 12, 1991, pp. 841-847. The main limitation of these biostable and biodegradable composites is their inadequate mechanical strength for large bone fracture fixation. Also, use of hydroxyapatite and poly lactic acid composites has been reported. See Y. Ikada, H.H. Suong, Y. Shimizu, S. Watanabe, T. Nakamura, M. Suzuki, A.T. Shimamoto, Osteosynthetic Pin, U.S. Patent 4,898,186, 1990. Using existing elements the composite still has quite moderate mechanical strength. Also in all these cases mentioned above the method of producing the composite differs from the method of the present invention.

10 Summary of the Invention

In this invention, we have established that the problems of inadequate strength and the brittleness of the bioactive bone fixation devices and the lack of bioactivity of absorbable polymeric devices are resolved by constructing a composite material comprising at least one resorbable polymeric matrix, at least one bioactive ceramic reinforcing element and at least one resorbable polymeric reinforcing component. The composite material described in more detail herein consists of two reinforcing components in a matrix material. One reinforcing element, the polymeric reinforcing element, is comprised of biodegradable polymer fiber and the other, called the ceramic reinforcing element, is comprised of bioceramic or bioglass.

- 15 Reinforced composite devices described in this invention have improved mechanical properties compared to non-reinforced devices, because reinforcement changes the behavior of material from brittle to ductile and thus makes device more reliable under load. Due to controlled manufacturing stages, mixing of matrix and ceramic reinforcing element as well as combining the polymeric reinforcing element, the

amount of both reinforcing element types is easily controlled. This is an important advantage, because the ratio of elements affects the mechanical properties of the device. Also, the amount of the ceramic reinforcing element affects the bioactivity of the device.

5

Brief Description of the Drawings

Figure 1 Shows a schematic picture of the cross-section of a composite plate of the invention.

Figure 2a Shows a FTIR spectrum of hydroxyapatite,

10 Figure 2b Shows a FTIR spectrum of hydroxyapatite-poly lactic acid composite, and

Figure 2c Shows a FTIR spectrum of poly lactic acid composite.

Description of the Preferred Embodiments

15 This invention relates to biodegradable materials used for bone fracture fixation devices and methods of their manufacture. Unlike other known materials used prior to this application, the composites of this invention have two different reinforcing phases and one matrix phase. One reinforcing element is referred as the polymeric reinforcing element and the other as the ceramic reinforcing element. The
20 matrix component can be any biodegradable or bioerodible polymer. Typical examples of these polymers are listed in Table 1 herein.

One reinforcing phase is a totally or at least partially oriented and/or fibrillated biodegradable or bioerodible polymer. This phase is called the polymeric reinforcing element, which is still recognizable and distinguishable from the final

product as a whole. The diameter of the reinforcing fibers can vary between 4 μm and 800 μm , preferably between 20 μm and 500 μm . Useful polymers for the polymeric reinforcing element include those listed in Table 1.

The ceramic reinforcing element can be comprised of a stable or a degradable
5 bioceramic or bioglass, or a mixture of these. Typical examples are listed in Table 2. They can be used in a powder, flake, spherical, fiber or any other form. Particle size can vary between 2 μm and 100 μm , preferably between 60 μm and 150 μm . In the case of fibers, the fibers are in all cases smaller than the polymeric reinforcing elements. The ceramic reinforcing element also acts as a bioactive, bony ongrowth
10 agent and provides a reservoir of calcium and phosphate ions, thus accelerating the healing time for bone fractures. While the matrix polymer degrades, bone can attach to the residual ceramic or glass particles. The amount of ceramic reinforcing element is 0.15 to 0.9 volume fraction, preferably between 0.2 and 0.6 volume fraction.

The defined particle size of the ceramic element in the composite described in
15 this invention is relatively big compared to conventionally used particle sizes for fillers or granules. In this invention, it was found unexpectedly that composites having bigger particle size ceramic elements are more biocompatible and cause less irritation to tissue than composites utilizing a ceramic element having small particle size. Biocompatibility is easily seen in histological studies. In tissue near and inside
20 the degrading composite implants having small ceramic particles there exists more giant cells than around and inside the degrading composite implants containing big (coarser) ceramic particles.

The invention may contain various additives and modifiers which improve the processability of the composite. Such additives include surface modifiers to improve

the attachment between the polymeric and ceramic components. The devices can also contain pharmaceutically active agent or agents, such as antibiotics, chemotherapeutic agents, wound-healing agents, growth hormones and anticoagulants (such as heparin). These agents are used to enhance the bioactive

5 feature of the composite and thus improve the healing process of the tissue.

Manufacture of the composite can be performed by any suitable plastics technology processing method. The matrix polymer and the ceramic reinforcing element(s) (bioceramic or bioglass) can be mixed together by powder mixing, melt mixing or solvent mixing. The polymeric reinforcing element (polymer fiber) can be

10 used as plain fiber or in modified form: for example, as braided or woven two or three dimensional structures. The mixture of matrix and the ceramic reinforcing element can be combined with the polymeric reinforcing element by melt mixing, by coating or by using solvent as an intermediate to preform the material (prepreg). The material can be produced in its final form by various techniques, including

15 compression molding, filament winding, mechanical machining or injection molding to any desired shape.

Due to controlled manufacturing stages, mixing of matrix and ceramic reinforcing element as well as combining the polymeric reinforcing element, the amount of both reinforcing element types is easily controlled. This is an important

20 advantage, because the ratio of elements affects the mechanical properties of the device. Also, the amount of the ceramic reinforcing element affects the bioactivity of the device. There should be sufficient bioceramic or bioglass to yield bony ongrowth.

Reinforced composite devices described in this invention have improved mechanical properties compared to non-reinforced devices, because reinforcement

changes the behavior of the material from brittle to ductile and thus makes the reinforced device more reliable under load. This feature is very important for load bearing applications, such as bone fracture fixation devices. For example, non-reinforced poly lactic acid devices typically have three-point bending strengths of 35-40 MPa and moduli of 3.5-4.0 GPa, and particulate reinforced (hydroxyapatite) poly lactic acid devices have values of 25-30 MPa and 5.0 GPa, respectively. Using polymer fiber reinforcement under the present invention, mechanical properties of two to five times higher are achieved.

10 EXAMPLES

The present invention is described in more detail by means of the following, non-limiting examples.

Example 1.

15 Plates sized approximately 50 x 10 x 2 mm were manufactured by compression molding from a powder mixture of poly (L,D-lactide) (95/5 L/D ratio) and hydroxyapatite with particle size of 60 μ m, reinforced unidirectionally with poly (L-lactide) fibers (53/35/12 weight percent of matrix polymer-hydroxyapatite - polymer fiber, respectively). Three-point bending strength (yield) and modulus were 20 69.8 MPa and 5.8 GPa, respectively, and no sample fracture was detected (ductile behavior). These results were compared to the results of similarly sized samples without fiber reinforcement, compression molded from (1) plain PLDLA 95/5 and from (2) powder mixture of PLDLA 95/5 and hydroxyapatite (60/40 w/w %). These samples showed three-point bending strengths (maximum) and moduli of (1): 38.0

MPa and 3.9 GPa and (2): 26.8 MPa and 5.0 GPa, respectively. These samples broke in bending without yielding, thus showing brittle fracture behavior.

Example 2.

- 5 Plates sized as in example 1 were manufactured by compression molding from a mixture of poly (L,D-lactide) (85/15 L/D ratio) and hydroxyapatite with particle size of 60 μ m reinforced unidirectionally with poly (L-lactide) fibers. Poly (L,D-lactide) and hydroxyapatite were previously melt mixed to a film for... The composition had 48/21/31 weight percent of matrix polymerhydroxyapatite-polymer
10 fibers, respectively. Three-point bending strength (yield) and modulus were 116.6 MPa and 6.1 GPa, respectively, and no sample fracture was detected.

Example 3.

- Plates sized approximately 50 x 10 x 1 mm were manufactured by
15 compression molding from the unidirectional prepreg material of poly (L,D lactide) (85/15 L/D ratio), hydroxyapatite and poly (L-lactide) fibers. The proportions of components varied from 3-16 wt-%, 15-50 wt-% and 48-85 wt-%, respectively. Three-point bending strength (yield) and modulus depended on the concentrations of the composite. Typical mechanical properties are listed in Table 3. No sample
20 fracture was detected and the behavior was ductile.

Table 3

	PLDLA (85/15) matrix (wt-%)	PLLA fibers (wt-%)	Hydroxy apatite (wt-%)	Three-point bending strength (MPa)	Three-point bending modulus (GPa)
5	3	82	15	136	9.5
	4	71	25	143	9.1
	5	47	48	141	12.2
	8	61	31	139	10.5
10	9	54	37	118	8.3
	16	48	36	166	9.6

Example 4.

- 15 Plates sized as in example 3 were manufactured by compression molding from a prepreg material of poly (L,D-lactide) (85/15 L/D ratio), hydroxyapatite and poly (L-lactide) fibers. The proportions of components were 4 wt-%, 15 wt-% and 81 wt-%, respectively. Three sample types were manufactured having different prepreg lay-ups of 0°/0°/0°/0°/0°, 0°/45°/0°/-45°/0° and 0°/0°/90°/0°/0°. Three-point bending
- 20 strengths (yield) and moduli were 135.9 MPa and 9.5 GPa, 140.1 MPa and 10.1 GPa, and 131.0 MPa and 9.3 GPa, respectively, and no sample fracture was detected.

Example 5.

- The surfaces of three different samples were studied by Fourier Transform
- 25 Infrared Spectroscopy. Samples were:

- a) hydroxyapatite
- b) hydroxyapatite-poly (D,L-lactide)-poly (L-lactide) composite

c) poly (D,L-lactide)-poly (L-lactide) composite.

The spectras from these samples are shown in figure 2. Matching peaks are detectable with samples b and c, which are poly lactide peaks. There also occur matching peaks from samples a and b which are characteristic of calcium phosphate compounds. The bioactivity of the composites claimed in this invention is the result of hydroxyapatite on the surface.

Example 6.

Plates sized as in example 3 were manufactured by compression molding from the unidirectional prepreg material of racemic poly (D,L-lactide), tricalcium phosphate with mean particle size of 70 μm and poly glycolide fibers. The proportions of components varied from 5 wt-%, 20 wt-% and 75 wt-%, respectively. Three-point bending strength (yield) and modulus were 195 MPa and 14.2 GPa, and no sample fracture was detected.

15

Example 7.

Plates sized as in example 3 were manufactured by compression molding from the prepreg material made of racemic poly (D,L-lactide), hydroxyapatite powder with mean particle size of 100 μm and the fabric made of poly (L-lactide) and poly (L,D lactide) (96/4) fibers. The proportions of components varied from 5 wt-%, 20 wt-% and 75 wt-%, respectively. Three-point bending strength (yield) and modulus were 150 MPa and 11.8 GPa, and no sample fracture was detected. Specimens showed similar mechanical properties in both the warp and the weft directions of the fabric.

Example 8.

Plates sized as in example 1 were manufactured by compression molding from a mixture of poly (ortho ester) and hydroxyapatite with mean particle size of 80 μm reinforced unidirectionally with poly (ortho ester) fibers. Poly (ortho ester) matrix and hydroxyapatite were previously melt mixed to a film form. The composition had 50/20/30 weight percent of matrix polymerhydroxyapatite-polymer fibers, respectively. Three-point bending strength (yield) and modulus were 105 MPa and 9.7 GPa, respectively, and no sample fracture was detected.

10 Example 9.

Plates sized as in example 3 were manufactured by compression molding from the unidirectional prepreg material of copolymer of poly (D,L lactide) and poly-e-caprolactone, tricalcium phosphate with mean particle size of 80 μm and poly-e-caprolactone fibers. The proportions of components varied from 16 wt-%, 30 wt-% and 54 wt-%, respectively. Three-point bending strength (yield) and modulus were 86 MPa and 3.4 GPa, and no sample fracture was detected. The strength and modulus values were lower than those for lactide based composites, but the extension to yield was much higher.

20

Example 10.

Plates sized as in example 1 were manufactured by compression molding from a mixture of a copolymer of poly (hydroxybutyrate)-poly (hydroxyvalerate) and a mixture of hydroxyapatite and tricalcium phosphate (50/50) with mean particle size

of 120 μm , reinforced unidirectionally with poly (hydroxybutyrate) fibers. The polymer matrix and ceramic mixture were previously melt mixed to a film form. The composition had 30/30/40 weight percent of matrix copolymer-ceramic mixture-polymer fibers, respectively. Three-point bending strength (yield) and modulus were 122 MPa and 6.2 GPa, respectively, and no sample fracture was detected.

Example 11.

Two set of samples (plates with 5 mm width, 20 mm length and 0.9 mm thickness) were implanted to the back of rats (subcurris). Specimens were made of poly-L lactic acid fibers, poly-D,L-lactic acid matrix (with L/D ratio 85/15) and hydroxyapatite powder using prepreg manufacturing method. The quantities of the components were 80 wt-%, 5 wt-% and 15 wt-%, respectively. The plates had five prepreg layers, with layer alignments of $0^\circ/0^\circ/0^\circ/0^\circ/0^\circ$. The mean particle diameter of hydroxyapatite powder in the first set of plates was 7.43 micrometers and in the second set of plates was 80 ± 20 micrometers.. The plates were gamma sterilized with a dose of 2.5 MRads.

Five animals from both sets were sacrificed after one year of implantation. In histological studies it was clearly seen, that in and around the composite plates with finer hydroxyapatite powder there existed significantly more giant cells than in the tissue of reference animals containing composite plates with coarser hydroxyapatite particles. Thus, coarser hydroxyapatite particles were shown to be more biocompatible.

TABLE 1. Resorbable polymers suitable for biocomposites.

Polymer

Polyglycolide (PGA)

Copolymers of glycolide:

Glycolide/L-lactide copolymers (PGA/PLLA)

Glycolide/trimethylene carbonate copolymers (PGA/TMC)

Poly lactides (PLA)

Stereocopolymers of PLA:

Poly-L-lactide (PLLA)

Poly-DL-lactide (PDLLA)

L-lactide/DL-lactide copolymers

Copolymers of PLA:

Lactide/tetramethylglycolide copolymers

Lactide/trimethylene carbonate copolymers

Lactide/d-valerolactone copolymers

Lactide/e-caprolactone copolymers

PLA/polyethylene oxide copolymers

Polydepsipeptides

Unsymmetrically 3,6-substituted poly-1,4-dioxane-2,5-diones

Poly-b-hydroxybutyrate (PHB)

PHB/b-hydroxyvalerate copolymers (PHB/PHV)

Poly-b-hydroxypropionate (PHPA)

Poly-p-dioxanone (PDS)

Poly-d-valerolactone
Poly-e-caprolactone
Methylmethacrylate-N-vinyl pyrrolidone copolymers
Polyesteramides
Polyesters of oxalic acid
Polydihydropyrans
Polyalkyl-2-cyanocrylates
Polyurethanes (PU)
Polyvinylalcohol (PVA)
Polypeptides
Poly-b-malic acid (PM LA)
Poly-b-alkanoic acids
Polycarbonates
Polyorthoesters
Polyphosphates

Table 2. Bioceramics and glasses suitable for biocomposites.

Hydroxyapatite
Tricalcium phosphate
Other calcium phosphates
Bioglass®
Ceravital®
Alumina

Zirconia

Bioactive gel-glass


Bioactive glasses

Alpha wollastonite glass ceramic

What is claimed is:

- 1 1. A biodegradable and bioactive composite material for surgical
2 osteosynthesis applications comprising: at least one resorbable polymeric matrix
3 component, at least one resorbable polymeric reinforcing element, and at least one
4 ceramic reinforcing element.

- 1 2. A method of manufacturing a biodegradable composite according to
2 claim 1, comprising the steps of:
3 a) selecting at least one first polymer for the matrix;
4 b) selecting at least one bioceramic for use as the ceramic reinforcing
5 element;
6 c) mixing said first polymer and said bioceramic together to form a
7 mixture;
8 d) selecting at least one second polymer in a fiber form;
9 e) placing said second polymer into a desired formation;
10 f) combining said mixture of step (c) and said formation of step (e) to
11 yield a second mixture; and
12 g) subjecting the second mixture of step (f) to heat or pressure.

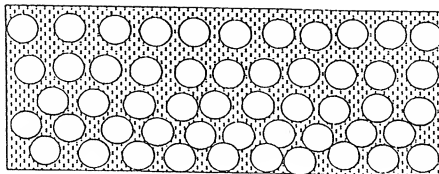


Fibrillated polymer reinforcement



Mixture of matrix polymer and bioceramic
or glass

FIG.1

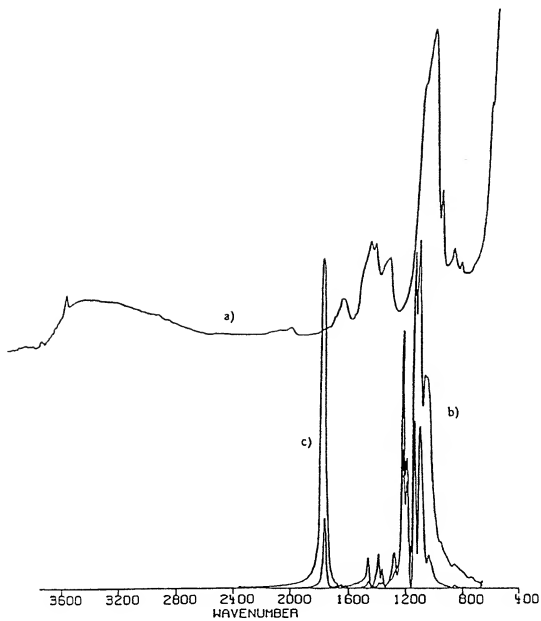FIG.2